


S1: (arrow marks) HRs >99.9 % @ 700 - 900 nm, AOI=45° (|GDDrs| < 20 fss)
S2: SCC

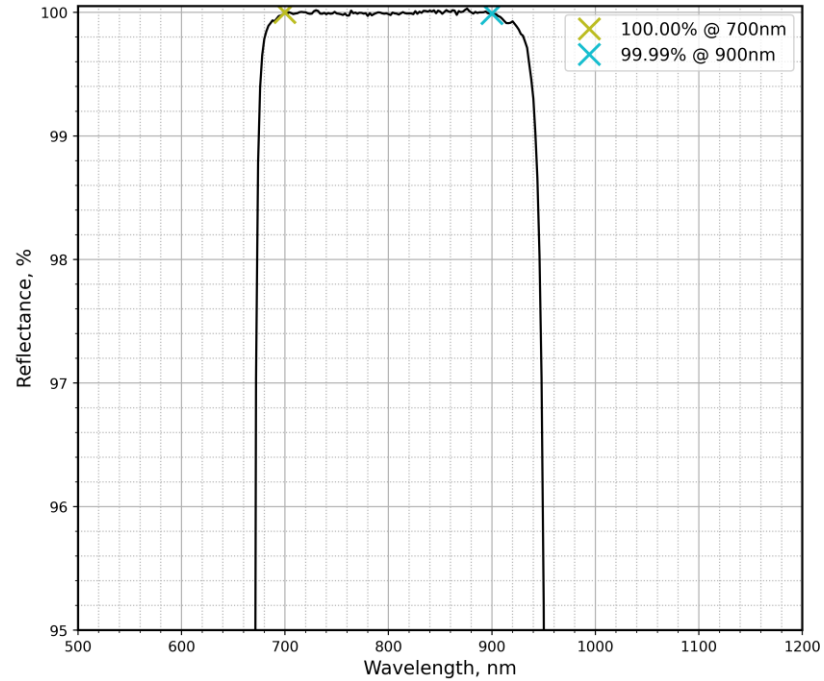

PO2818 Rs i45

Fig. 1.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%